




**Product Specification**  
**Micro sample tube Fluoride/heparin FH, 1.3 ml,  
screw cap, ISO**

**Page 1**

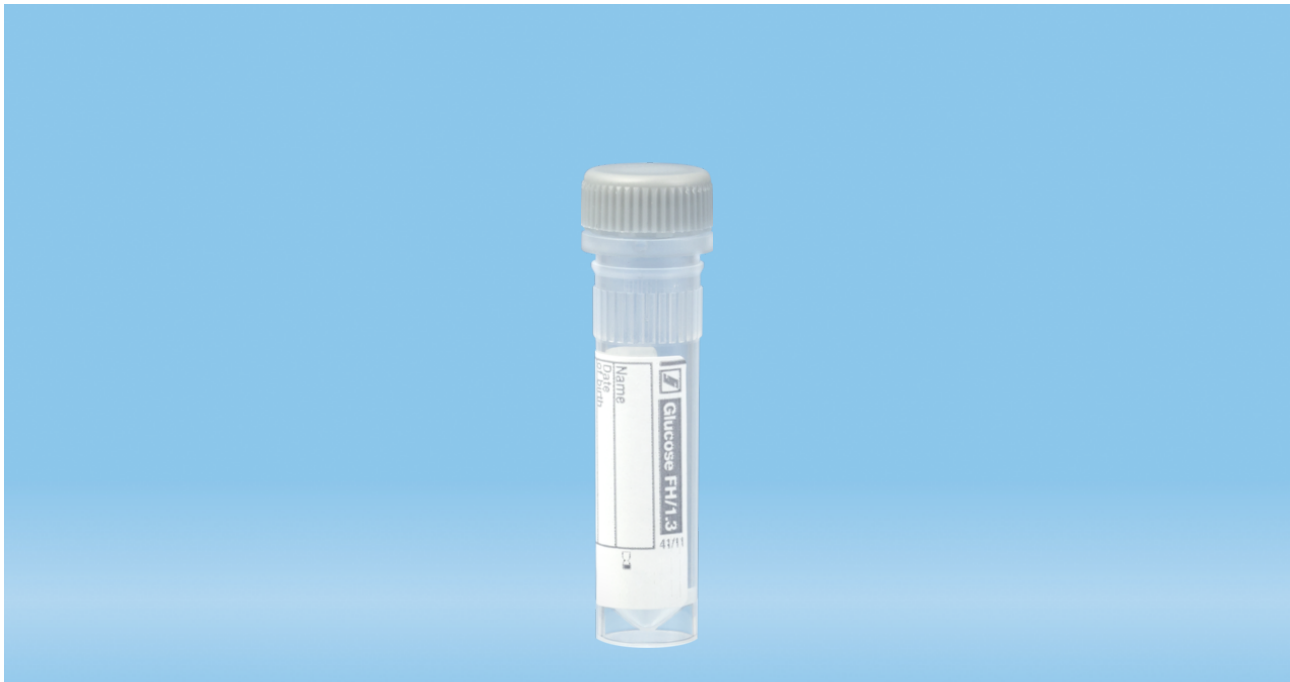

**Product description**

Order number	41.1394.105
Product description	Micro sample tube Fluoride/heparin FH, venous blood collection, preparation: Fluoride + heparin, nominal volume: 1.3 ml, (LxØ) with cap: 47 x 10.8 mm, screw cap, cap: grey, colour code ISO, with paper label, label/print: grey, skirted conical base, 100 piece(s)/bag

**Product characteristics**

Type of collection	venous
Type of preparation	Fluoride + heparin
Preparation concentration	1.0 mg/ml blood + 16 IU/ml blood
Colour code	ISO
Label/ Print	with paper label
Colour of print/label	grey
Graduation	yes
Closure type	screw cap
Application	venous blood collection
Base shape	skirted conical base
Volume of work	1,3 ml

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.





**Product Specification**  
**Micro sample tube Fluoride/heparin FH, 1.3 ml,  
screw cap, ISO**

**Page 2**

Recommended centrifugation 2000 x g  
Centrifugation time 5 Min

**Size**

Sample volume 1.3 ml  
Diameter 10.8 mm  
Length of product 47 mm  
Length including cap 47 mm  
Length excluding cap 45 mm

**Material & colours**

Colour of product transparent  
Closure material Polypropylene (PP)  
Colour of cap grey  
Tube material Polypropylene (PP)

**Purity & certification**

Satisfies the requirement IATA, ADR  
Product category In vitrodiagnostic device, CE  
CE certified CE  
Batched yes

**Packaging**

Minimum order qty. 1000  
Type of smallest bag  
subpackaging  
Piece(s) / inner box 100  
Piece (s) / outer case 1000  
Piece(s) / pallet 96000  
Depth of case 348 mm  
Width of case 278 mm  
Height of case 140 mm  
Case volume 0.0135 cbm  
Weight of product 0.0016 kg  
Weight of case 1.91 kg  
EAN of inner box 4038917128353  
EAN case 4038917021678

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

Date of issue:  
2024-07-03

This document was prepared by EDP support and is valid without signature.



**SARSTEDT**