




## Product Specification

PCR plate without skirt, 96 well, white, High Profile, 200 µl, PCR Performance Tested, PP

Page 1

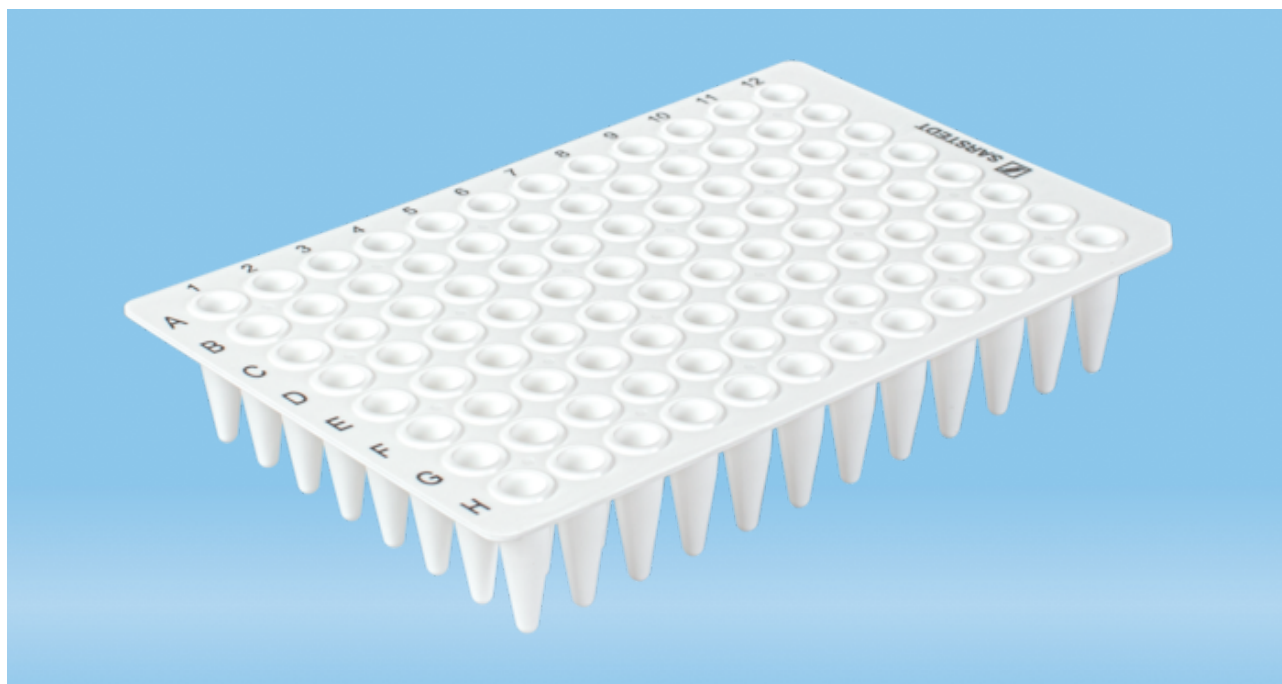

### Product description

Order number	72.1978.010
Product description	PCR plate without skirt, 96 well, white, High Profile, 200 µl, PCR Performance Tested, material: PP, optimised for qPCR, 10 piece(s)/minigrip bag

### Product characteristics

Closure type	film
Suitable for qPCR	yes
Base shape	conical
Construction of the plate edges	without skirt
High or low profile	High Profile
Number of wells	96
Volume of work	2 µl - 200 µl
Centrifugation max (RCF)	3000 x g
Centrifugation temperature	22
Centrifugation time	5 Min
Autoclavable (max. °C)	121 °C

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

Date of issue:  
2024-06-30

This document was prepared by EDP support and is valid without signature.



**SARSTEDT**



## Product Specification

**PCR plate without skirt, 96 well, white, High Profile, 200 µl, PCR Performance Tested, PP**

**Page 2**

### Size

Sample volume	0.2 ml
Max. volume	200 µl
Diameter	5.51 mm
Width of product	76 mm
Height of product	21 mm
Length of product	119.9 mm

### Material & colours

Product material	Polypropylene (PP)
Colour of product	white

### Purity & certification

Product category	no medical device   IVD
Purity standard	PCR Performance Tested
Batched	yes

### Packaging

Minimum order qty.	100
Type of smallest subpackaging	minigrip bag
Piece(s) / inner box	50
Piece (s) / outer case	100
Piece(s) / pallet	5600
Depth of box	270 mm
Width of box	230 mm
Height of box	131 mm
Depth of case	282 mm
Width of case	280 mm
Height of case	247 mm
Case volume	0.0195 cbm
Weight of product	0.0165 kg
Weight of case	2.27 kg
EAN of inner box	4038917557665
EAN case	4038917557658

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

Date of issue:  
2024-06-30

This document was prepared by EDP support and is valid without signature.



**SARSTEDT**